
2019-nCoV IgM/IgG Antibody Test Kit

Liquid Phase



((

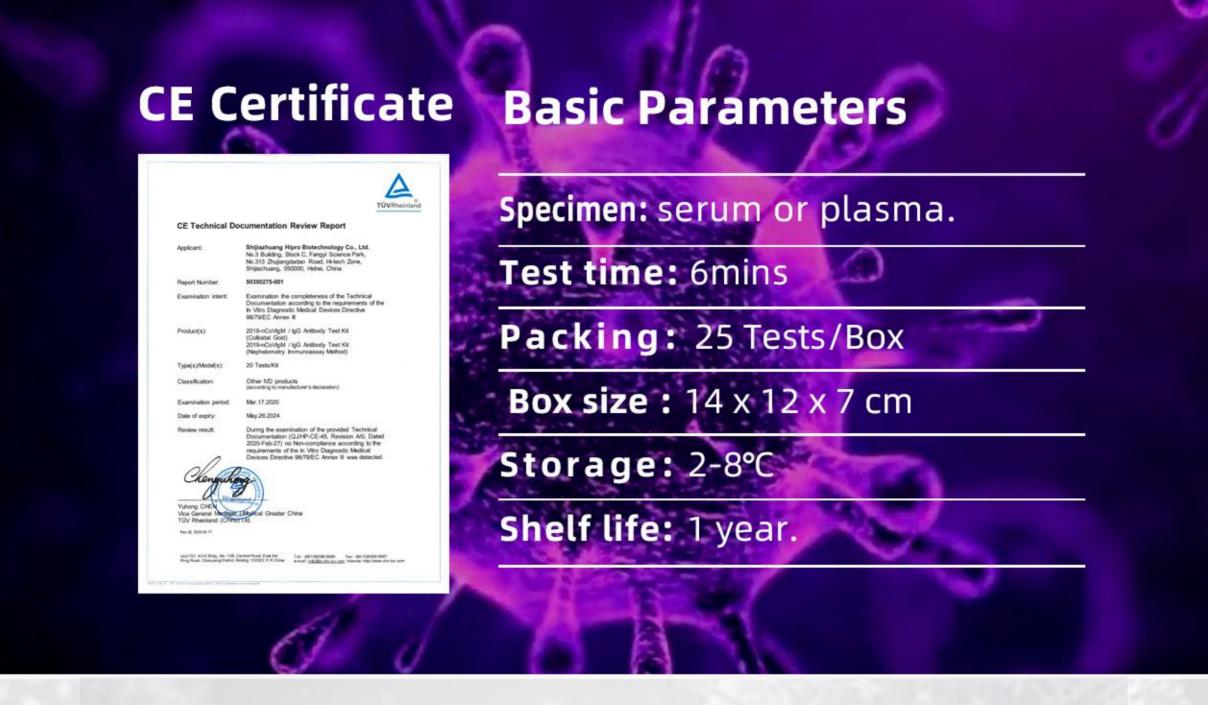

Accurate

• React in liquid phase

Precisely quantitative sample collection

- High specificity and High sensitivity
 Avoid false negative and false positive

Safe

• Protect operator from contact with samples

Works with serum, & plasma

V.

Fast

• 6 minutes per test

Results displayed in numbers

Steps



Immunoassay System



Immunoassay System

Immunoassay System

Negative:Test result<0.5ng/ml

Positive:Test result > 0.5 ng/ml

It was recommended to use nCoV-IgM /IgG to specifically detect the antibodies of the novel coronavirus (2019-ncov) in the blood, to exclude fever cases caused by other viruses, or to diagnose the 2019-nCoV infection. After the human body was infected with the novel coronavirus, human body


would produce corresponding antibodies, IgM comes

first. When IgM production declines, IgG production is

accelerated to cope with the invasion of pathogens.

Antibody Test ¦ IgM ; ← IgM+IgG -

Clinical application

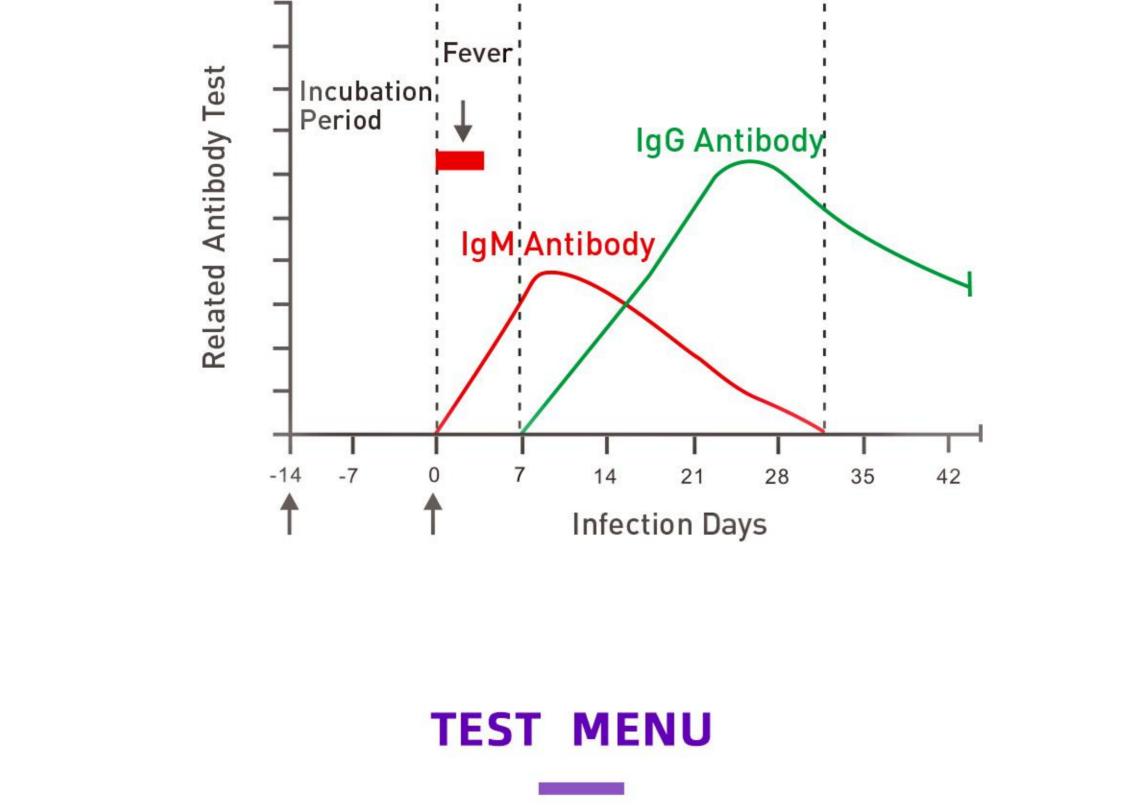

PCT H-FABP Full range CRP Myo SAA cTnl

Infection

Cardiovascular disease

Rheumatism

ASO

CRP

| SAA | cTnI | Anti-CCP |
|-------------------------------------|----------------------------------|--|
| Renal-Function | HCY | RF |
| HbA1C | NT-proBNP | Autoimmunity |
| Cys-C | Lp(a) | IgA |
| mAlb | Lp-PLA2 | IgG |
| NGAL | CK-MB | IgM |
| RBP | D-Dimer | IgE |
| α 1 – MG | Gastric Function | Hormones |
| β2-MG | ★ HP | HCG |
| i a | | |
| Microelement | PGI | ★ LH |
| Microelement 25-OH-VD | PGI | Thyroid Function |
| | | |
| 25-OH-VD | PGII | Thyroid Function |
| 25-OH-VD FER | PGII Tumor Marker | Thyroid Function |
| 25-OH-VD FER Liver Function | PGII Tumor Marker AFP | Thyroid Function ★ T3 ★ T4 |
| 25-OH-VD FER Liver Function ADA | PGII Tumor Marker AFP CEA | Thyroid Function ★ T3 ★ T4 ★ TSH |
| 25-OH-VD FER Liver Function ADA TRF | PGII Tumor Marker AFP CEA PSA | Thyroid Function ★ T3 ★ T4 ★ TSH ★ FT3 |



Hipro Biotechnology Co., Ltd